

# Potentiometric Selectivity

*by* Asep Saefurrohman

---

**Submission date:** 19-Apr-2023 02:54AM (UTC+0700)

**Submission ID:** 2068634450

**File name:** AIP\_Paper\_ICMNS\_ASEP\_SAEFUROHMAN.docx (51.46K)

**Word count:** 2444

**Character count:** 13859

# Potentiometric Selectivity Of Polymer-Membrane Electrodes Based On Lanthanum

Asep Saefurohman<sup>1\*</sup>, Buchari<sup>1</sup>, Indra Noviani<sup>1</sup>, Syoni<sup>2</sup>

<sup>1</sup> Department of Chemistry, Bandung Institute of Technology, Indonesia

<sup>2</sup> Department of Material Engineering, Bandung Institute of Technology, Indonesia

\* Email: saefurohman.asep78@Gmail.com

**Abstract.** Quantitative analysis of rare earth elements which are considered as the standard method that has a high accuracy, and detection limits achieved by the order of ppm is inductively coupled plasma atomic emission spectroscopy (ICPAES). But these tools are expensive and valuable analysis of the high cost of implementation. In this study be made and characterized selective electrode for the determination of rare earth ions is potentiometric. Membrane manufacturing techniques studied is based on immersion (liquid impregnated membrane) in PTFE 0.5 pore size. As ionophores to be used tributyl phosphate (TBP). There is no report previously that TBP used as ionophore in polymeric membrane based lanthanum. Some parameters that affect the performance of membrane electrode such as membrane composition, membrane thickness, and types of membrane materials studied in this research. Manufacturing of Ion Selective Electrodes (ISE) Lanthanum (La) by means of impregnation La membrane in TBP in kerosene solution has been done and showed performance for ISE-La. FTIR spectrum results for PTFE 0.5 pore size which impregnated in TBP and PTFE blank showed difference of spectra in the top 1257 cm<sup>-1</sup>, 1031 cm<sup>-1</sup> and 794.7 cm<sup>-1</sup> for P = O stretching and stretching POC from group -OP = O. The result showed shift wave number for P = O stretching of the cluster (-OP=O) in PTFE-TBP mixture that is at the peak of 1230 cm<sup>-1</sup> indicated that no interaction bond between hydroxyl group of molecules with molecular clusters fosforil of TBP or R<sub>3</sub>P = O. The membrane had stable responses in pH range between 1 and 9. Good responses were obtained using 10<sup>-3</sup> M La(III) internal solution, which produced relatively high potential. ISE-La showed relatively good performances. The electrode had a response time of 29±4.5 second and could be use for 50 days. The linear range was between 10<sup>-5</sup> M and 10<sup>-1</sup>

**Keywords:** You should enter keywords here (in a single line length).

**PACS:** 15

## INTRODUCTION

Rare earth elements is known as an important element of their nature, especially having a strong magnetic properties. Rare earth elements found in nature in the form of minerals such as monazite. Monazite is one mineral that contains lots of rare earth metal element (REE') of the lanthanide group. This mineral also found in Indonesia, but not yet processed and utilized optimally because of the mastery of monazite ore processing technology still needs to be improved and strengthened. REE' these elements, are now widely used for the manufacture of goods innovative high-tech, such as permanent magnets, catalysts, fiber optics, optoelectronics, ceramics pizeoelectric, rechargeable batteries, microwave equipment, etc., so that now the element REE has regarded as one of the 21st century (Morais and Cimenelli, 2004). But the element of REE' mostly have physical and chemical properties are similar, making it hard splitting into each element. It is also the cause of rare earth metals such as lanthanides become expensive (Shimojo *et.al.*, 2007).

17  
Currently, many researchers who give great attention to rare earth metals are widely applied in industry. Therefore, the required development of methods for the determination and recovery of rare earth metals. Method has been developed which includes conventional means such as chemical precipitation, reverse osmosis, adsorption, ion exchange and solvent extraction, but many difficulties are found in a variety of methods (Darviche *et.al.*, 2008). For the purposes of monitoring the treatment process, quality control, and REE' presence in a given material, required analytical methods that have high accuracy and selectivity, low detection limits, and high reproducibility. The method is considered to meet these criteria, among others, spectroscopic techniques such as inductively coupled plasma mass spectrometry (ICPMS), inductively coupled plasma atomic emission spectrometry (ICPAES), and X-ray fluorescence spectrometry (Houk *et.al.*, 1980; Anonymous, 1988). Hence, the available methods for low-level determination of rare-earth ions in solution include spectrophotometry, isotope dilutions mass spectrophotometry, neutron activation analysis, X-ray fluorescence spectrometry, etc (Mittal, *et.al.*, 3003). However, many of these spectroscopic methods requires a lot of time involving multiple samples and

also expensive for most analytical laboratories (Faridbod *et al.*, 2008). Meanwhile, if using chromatographic methods require a long sample preparation. Therefore, alternative methods are needed that meet the analytical criteria, simple in execution and relatively inexpensive. One method that has the potential of the electrode is the potentiometric method with membranous. Potentiometric method provides several advantages such as speed and ease of preparation and procedures, simple instrumentation, relatively fast response, very low detection limits, wide measurement range, an acceptable selectivity and low cost. This will make the availability of micro-electrodes and electrodes for the determination of the required REE (Ganjali *et al.*, 2007). Membranous electrode has many types, and in this paper was chosen with reference to the type of tube and the solution in as well as sensor ionophores required. Therefore, it is feasible the development of methods to make sensors for lanthanide ions with high selectivity using the appropriate ionophores.

Electrodes for the potentiometric determination can yield several benefits such as ease and speed of preparation and procedures, simple instrumentation, relatively fast response, wide measurement range and low cost. Therefore, the use of microelectrode and an electrode in the potentiometric analysis REE' is growing. Meanwhile, the transport mechanism in the impregnated liquid membrane (ILM) and the bulk membrane (BM) is based on the price Coefficient of distribution of the species are transported in membrane and solution interfaces (external and internal). With reference to the extraction solvent has managed quite well for the extraction of REE' with supported liquid membrane (SLM) using organophosphate compounds such as TBP, TOPO, and EHEHP D<sub>2</sub>EHP. Hence, in this paper the compound will be studied or used as ionophores in membranes in selective electrodes ion. The principle of formation of the measured potential in both surface and transport based on this principle the same as that occurs in the extraction, while the TBP solvent extraction and D<sub>2</sub>EHPA lanthanides have been performed and shown to occur transport from the aqueous phase to organic phase by using TBP and D<sub>2</sub>EHPA. In addition, both compounds have not been used as ionophores in potentiometric systems.

Method for making membranes as sensors developed at this time both have advantages and disadvantages. The advantages in terms of preparation ILM is easier, faster transport, and from the aspect of mobility at the ILM ionophores higher while the lack of ILM is the leakage rate during the experiments ionophores higher. Meanwhile, the excess solvent and BM is the arrangement of ionophores fused with the membrane material, so that the evaporation time strongly retained

ions in the membrane structure, but the mobility of ionophores on the BM is slower because more meetings/densed and shorter trajectory measurements. To study the character of the membrane on the electrode as a potentiometric sensor, needed characterization, membrane potential, response time, sensitivity, selectivity towards the primary ion and ion bullies are less than 10<sup>-3</sup>, age (lifetime) is relatively long and has a design size can be miniaturized.

The main objective of this work is to introduce a selective and sensitive electrode for lanthanum, for the potentiometric monitoring of trace amount of La<sup>3+</sup>, Gd<sup>3+</sup>, and Yb<sup>3+</sup> by using D<sub>2</sub>EHPA and TBP as ionophore and its applications for measurement of monazite and bentonite ore from Bangka Belitung island and compare with standard method of ICP-AES.

## MATERIAL AND METHOD

### MATERIALS

Di-(2-ethylhexyl) phosphoric acid and tributyl phosphate were obtained from Sigma Aldrich. High molecular weight poly(vinyl chloride), potassium tetrakis (4-chlorophenyl) borate (KTCPB), o-nitro phenyl octyl ether (NPOE), PTFE (Advantec, Japan) with pore size 0,45  $\mu\text{m}$  pore and 0,2  $\mu\text{m}$  pore. All other reagents used were of analytical grade and the solutions were prepared in doubly distilled water.

### Potential Measurement

The potential measurements of the solutions, prepared in the concentration range  $1.0 \times 10^{-1}$  -  $1.0 \times 10^{-6}$  M La<sup>3+</sup>, Gd<sup>3+</sup>, and Yb<sup>3+</sup> ions, were carried out at  $25 \pm 1$  °C with a Keithly 6  $\frac{1}{2}$  instrument pH/Ion meter. Leakless Ag/AgCl electrode (EDAQ) were employed as reference electrodes and potential were measured by setting up the following assembly:  
Internal Reference electrode | internal | solutions  
Membrane | Test Solutions | External reference electrode

### Membrane and Electrode Preparation

The method reported by Suyanta *et al.*, 2006 and Jain A.J *et al.*, (1998) was adopted for the fabrication of membranes. Membrane prepared in two method, Impregnated Liquid membrane (ILM) and bulk membrane (BM). Impregnated Liquid membranes used for prepared ESI-La, with Teflon, length 10 cm, 1,5 diameter. PTFE (Advantec, Japan) with pore size 0,45  $\mu\text{m}$  pore and 0,2  $\mu\text{m}$  pore (impregnated in TBP and D<sub>2</sub>EHPA), for 12 and 24 hours respectively. Bulk

membranes was prepared by dissolving varying amounts (10 -100 mg), PVC, NPOE and KTCPB in THF. The solution was evaporated on a plane glass with an area of  $1.5 \times 4 \text{ cm}^2$ . The electrode was prepared by glueing the electrode tube to the membrane. The inner reference electrode Ag/AgCl and the inner solution (a mixture of  $10^{-3} \text{ M KCl}$  and  $10^{-3} \text{ M La}^{3+}$ ) was set in the tube and connected to coaxial cable. The electrode was conditioned before potentiometric measurement by immersing it into  $10^{-3} \text{ M LaO}_3$  solution for 24 hours. The homogeneous mixture was poured into glass rings placed on smooth glass plates and the solvent was allowed to evaporate overnight, yielding a membrane of about 0.5 mm thickness and 10 mm diameter. A number of membranes of different compositions were prepared and only those which gave reproducible and stable potentials were selected for further studies.

## 21 RESULT AND DISCUSSION

### Working Concentration Range and Slope

The potential response of all the three electrode using PTFE membrane 0.45  $\mu\text{m}$  pore size with TBP in kerosene was investigated by varying the concentration of the test solution from  $1.0 \times 10^{-1}$  -  $1.0 \times 10^{-6}$ .

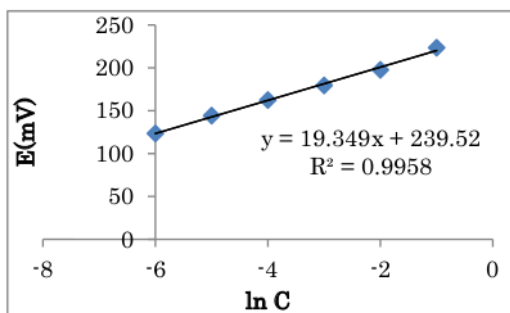


FIGURE 1. Curve calibration for Electrode 3

The electrodes 3 is impregnated in TBP exhibit linear potential response in the concentration range  $1.5 \times 10^{-1}$  -  $1.0 \times 10^{-6}$  with a ideal-Nernstian slope of 19.34 mV per decade activity. Meanwhile, electrodes 1 and electrodes 2 exhibit linear potential in the concentration range  $2.5 \times 10^{-1}$  -  $1.0 \times 10^{-6}$  and  $2 \times 10^{-1}$  -  $1.0 \times 10^{-6}$  with near-Nernstian slope 15.44 and 18.66 mV per decade activity, respectively. It is important to mention that the addition of plasticizers did not improve the performance of the membranes. This observation may be ascribed to the fact that D2EHPA and TBP themselves act as plasticizers and have been used earlier for this purpose (Jain *et al.*, 1998).

### Response Time and Performance of Electrodes

## IR Spectra

The spectrum results for PTFE 0.2 pore size which impregnated in TBP and PTFE blank showed difference of spectra in the top  $1257 \text{ cm}^{-1}$ ,  $1031 \text{ cm}^{-1}$  and  $794.7 \text{ cm}^{-1}$  for P=O stretching and stretching POC from group -OP=O. The result showed shift wave number for P=O stretching of the cluster (-OP=O) in PTFE-TBP mixture that is at the peak of  $1230 \text{ cm}^{-1}$  indicates that no interaction bond between hydroxyl group of molecules with molecular clusters fosforil of TBP or  $\text{R}_3\text{P} = \text{O}$ .

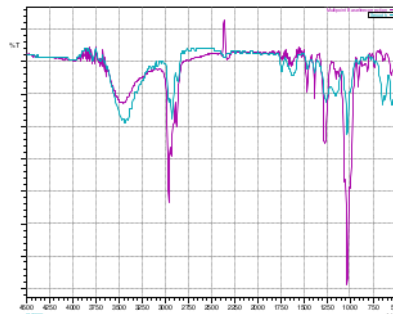
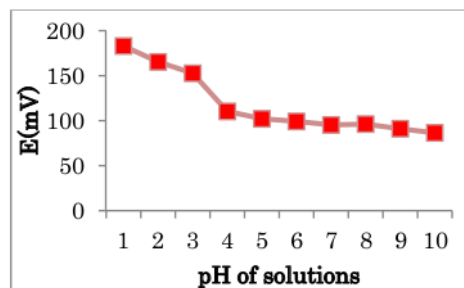


Figure 2. Spektrum FTIR for ESI-La impregnated membrane TBP

## 36 Effect of pH on the Potential Response

A series of solutions of  $\text{La}^{3+}$  with pH ranging from 1 to 10 were prepared by adding  $\text{H}_2\text{SO}_4$  and NaOH solutions. Solution potentials were measured by the cell system. pH dependence of the membrane electrode was investigated at  $1.0 \times 10^{-3} \text{ M La}^{3+}$  concentration in the pH range 1-10 by adjusting the pH solution with  $\text{H}_2\text{SO}_4$  and NaOH. It was observed that the potential remains constant in the pH range relatively 4-9 and the same was taken as the working pH range of the electrodes. These results were relatively the same as those reported by other researchers, stating that pH was kept constant at 3-8 (Suyanta *et al.*, 2006) and 3-9 (Ganjali *et al.*, 2004; Gadzeppo and Christian, 1984).



**TABLE 1. Performance of TBP-PTFE membrane sensor**

Electrode Number	Slope mV/decade	Working concentration	R <sup>2</sup>
Electrode 1	15.44	2.5×10 <sup>-1</sup> -1.0×10 <sup>-6</sup>	0.9960
Electrode 2	18.66	2×10 <sup>-1</sup> -1.0×10 <sup>-6</sup>	0.9990
Electrode 3	19.34	1.5×10 <sup>-1</sup> - 1.0×10 <sup>-6</sup>	0.9950

From the table 1 its seen the potential response of all the three electrodes using membranes of PTFE and TBP of different composition was investigated by varying the concentration of the test solution from 105×10<sup>-1</sup>-1.0×10<sup>-6</sup>. The results obtained are given in Table 2 for the response time each electrode. It is seen that the electrodes nos. 1 and 2 having membranes of exhibit linear potential response in the concentration. Range but slope are closely to Nernstian-law. The table 2 shown response time of electrode 1, 2, and 3 respectively. Its seen that electrode 3 has the faster response comparing with electrode 1 and 2.

**TABLE 2.** Response time of electrodes

Electrode Number	Composition	Response time
Electrode 1	PTFE-TBP	30
Electrode 2	PTFE-TBP	31
Electrode 3	PTFE-TBP	29.45

## CONCLUSIONS

Among the three PTFE impregnated membrane, the ones having good performance with regard to the working electrodes and shown Nernstian slope 19.34 mV per decade activity.

## ACKNOWLEDGMENTS

Author thanks goes to the Postgraduate scholarship program DIKTI Ministry of education and culture of Indonesia for funds provided to conduct research at the Institute for Chemie, Department of Analytical Chemistry -ITB.

## REFERENCES

1. Attas, A. Novel PVC membrane selective electrode for the determination of clozapine in pharmaceutical preparation. *Int. J. Electrochem. Sci.* 9-19.(2009).
2. Baker, E *et al.* Carrier-baed ion selective electrodes and bulk optodes, ionophores for potentiometric and optical sensors. *Chem Rev.*, 98:1593-1687. (1998).
3. Chowdhury D.A, Ogata T. Dan Kamato S. Samarium (III) selective electrodes using neutral bis (thiaalkylxanthato) alkanes. *Anal.Chem.*62, 366-378. (1996).
4. Darviche, *et al.*. Lanthanide recognition: A Ho<sup>3+</sup> Potentiometric membrane sensor. *Int J. Electrochem.Sci* Vol 3:1288-1298.(2008).
5. Faridbod, *et al.*. The fabrication of potentiometric membrane sensors and their application. *African Journal of Biotechnology.* 6, 25, 2967-2987. (2008).
6. Ganjali M.R., *et al.* Ppt levels detection of samarium (III) with a coated graphite sensor based on an antibiotic, *Analytical Sciences*, 20, 1007-1011. (2007).
7. Ito, K, Goto, C and Noguchi, K. Lanthanoid ion selective solvent polymeric membrane electrode based on 1-phenyl-3-methyl-4-octadecanoyl-5-pyrazolone. *Analytica Chimica Acta.* Vol 443:41-51.( 2001).
8. Mittal, S.K., Kumar S.K.,and Sharma,H.K PVC-Based dicyclohexano-18-crown-6 sensor for La(III) ions. *Talanta*, 62, 801-805. (2004).
9. Morais, CA dan Ciminelli, V.S.T. Process development for the recovery of High-grade lanthanum by solvent extraction. *Hydrometallurgy*, 73, 237- 244.(2004).
10. Norouzi *et al.*, Novel neodymium (III) membrane sensor based on N-(2-Furylmethylene) pyridine-2,6-diamine. *J. Braz. Chem. Soc.*, Vol.17:1-7. (2006).
11. Shamsifur, M *et al.* . PVC-Based 1,3,5-Trithiane sensor for cerium(III) ions. *Anal.Chem.*, Vol 72:2391-2394. (2000).
12. Shimojo, K, Naganawa, H, Noro, J and Kubota, F.. Extraction Behaviour and separation of lanthanides with a diglycol amic Acid Derivative and a Nitrogen-donor Ligand. *Analytical Sciences*, Vol 23.1427-1430. (2007).
13. Suyanta, *et al.* Lanthanum (III) selective Electrode Based on 1,10-Diaza-4,7 13, 16 tetraoxacyclooctadecane-N,N'-Diacetic Acid (DACDA) as an ionophore. Ph.D thesis. 2006.

# Potentiometric Selectivity

---

## ORIGINALITY REPORT

---

23%

SIMILARITY INDEX

15%

INTERNET SOURCES

20%

PUBLICATIONS

%

STUDENT PAPERS

---

## PRIMARY SOURCES

---

1

[www.researchgate.net](http://www.researchgate.net)

Internet Source

2%

---

2

Mohammad Reza Ganjali, Parviz Norouzi, Behrouz Akabri - Adergani, Siavash Riahi, Bagher Larijani. "An Asymmetric Lutetium(III) Microsensor Based on N - (2 - Furylmethylene) Pyridine - 2,6 - Diamine for Determination of Lutetium(III) Ions", Analytical Letters, 2007

Publication

1%

---

3

Vinod K Gupta. "A PVC-based 12-crown-4 membrane potentiometric sensor for zinc (II) ions", Sensors and Actuators B: Chemical, 1999

Publication

1%

---

4

Abreu, R.D.. "Purification of rare earth elements from monazite sulphuric acid leach liquor and the production of high-purity ceric oxide", Minerals Engineering, 201005

Publication

1%

---

5	Gupta, Vinod Kumar, L.P. Singh, Rakesh Singh, N. Upadhyay, S.P. Kaur, and Bhavana Sethi. "A novel copper (II) selective sensor based on Dimethyl 4, 4- $\text{O}^2$ (o-phenylene) bis(3-thioallophanate) in PVC matrix", Journal of Molecular Liquids, 2012.	1 %
Publication		
6	Vinod Kumar, Rishi Suri, Sachin Mittal. "Review on new ionophore species for membrane ion selective electrodes", Journal of the Iranian Chemical Society, 2022	1 %
Publication		
7	Gupta, V.K.. "Manganese (II) selective PVC based membrane sensor using a Schiff base", Talanta, 20070415	1 %
Publication		
8	Gupta, V.K.. "PVC-based neutral carrier and organic exchanger membranes as sensors for the determination of $\text{Ba}^{2+}$ and $\text{Sr}^{2+}$ ", Sensors & Actuators: B. Chemical, 19990511	1 %
Publication		
9	Ganjali, M.R.. "Ytterbium(III)-selective membrane electrode based on cefixime", Analytica Chimica Acta, 20030103	1 %
Publication		
10	S Mittal. "PVC-based dicyclohexano-18-crown-6 sensor for La(III) ions", Talanta, 2004	1 %
Publication		

11	<a href="http://onlineservices.ipophil.gov.ph">onlineservices.ipophil.gov.ph</a> Internet Source	1 %
12	Hassan Ali Zamani, Mahbobeh Mohaddeszadeh. "Determination of Dysprosium(III) Ion in Soil and Sediment Samples by an Original Potentiometric Dysprosium(III) Membrane Sensor", <i>Analytical Letters</i> , 2008 Publication	1 %
13	<a href="http://warwick.ac.uk">warwick.ac.uk</a> Internet Source	1 %
14	GUPTA, Vinod Kumar, Rainer LUDWIG, and Shiva AGARWAL. "Strontium(II) Sensor Based on a Modified Calix[6]arene in PVC Matrix", <i>Analytical Sciences</i> , 2005. Publication	1 %
15	<a href="http://garuda.kemdikbud.go.id">garuda.kemdikbud.go.id</a> Internet Source	1 %
16	<a href="http://www.tandfonline.com">www.tandfonline.com</a> Internet Source	1 %
17	PEI, L.. "Separation of Eu(III) with supported dispersion liquid membrane system containing D2EHPA as carrier and HNO <sup>3</sup> solution as stripping solution", <i>Journal of Rare Earths</i> , 201101 Publication	1 %



- |    |   |      |
|----|---|------|
| 18 | <a href="http://sciencejournals.ru">sciencejournals.ru</a><br>Internet Source   | 1 %  |
| 19 | Mohammad Reza Ganjali, Parviz Norouzi, Taher Alizadeh, Azadeh Tajarodi, Younes Hanifehpour. "Fabrication of a highly selective and sensitive Gd(III)-PVC membrane sensor based on N-(2-pyridyl)-N'-(4-nitrophenyl)thiourea", <i>Sensors and Actuators B: Chemical</i> , 2007<br>Publication | <1 % |
| 20 | <a href="http://accedacris.ulpgc.es">accedacris.ulpgc.es</a><br>Internet Source   | <1 % |
| 21 | <a href="http://docshare.tips">docshare.tips</a><br>Internet Source   | <1 % |
| 22 | "PVC Membrane Sensor for Nd (III) Based on N 1 , N 2 -Bis (Salicylidine) Butane-1, 4 - Diamine", <i>International Journal of Advanced Research in Chemical Science</i> , 2016<br>Publication  | <1 % |
| 23 | Ashok Kumar Singh, Puja Saxena, Amit Panwar. "Manganese(II)-selective PVC membrane electrode based on a pentaazamacrocyclic manganese complex", <i>Sensors and Actuators B: Chemical</i> , 2005<br>Publication  | <1 % |
| 24 | Gupta, V.K.. "Electroanalytical studies on cobalt(II) selective potentiometric sensor   | <1 % |

based on bridge modified calixarene in poly(vinyl chloride)", *Electrochimica Acta*, 20080630

Publication

---

25

Kefira Sutanto, Ari Widyanti, Gradiyan Budi Pratama, Herman R. Soetisna. "Technology for reducing distracted driving in developing countries: the level of usage and intention to use in Indonesia", *Heliyon*, 2022

Publication

---

26

Mohamed B. Saleh, Ahmed A. Abdel Gaber, Moustafa M.R. Khalaf, Ahmed M. Tawfeek. "A new ion-selective electrode for potentiometric determination of Ce(III) ions", *Sensors and Actuators B: Chemical*, 2006

Publication

---

27

Rui A. S. Lapa, José L. F. C. Lima, M. H. Vela, E. Barrado. "Sequential Determination of Calcium and Magnesium Cations in Haemodialysis Solutions by FIA", *Analytical Sciences*, 1997

Publication

---

28

[www.mdpi.org](http://www.mdpi.org)

Internet Source

---

29

[www.semanticscholar.org](http://www.semanticscholar.org)

Internet Source

---

<1 %

<1 %

<1 %

<1 %

<1 %

30 A. K. Jain. "A new membrane sensor for UO<sub>22+</sub> ions based on 2-hydroxyacetophenoneoxime-thiourea-trioxane resin", *Electroanalysis*, 07/1997  
Publication <1 %

---

31 A.K. Jain, V.K. Gupta, R.D. Singh, U. Khurana, L.P. Singh. "Nickel(II)-selective sensors based on heterogeneous membranes of macrocyclic compounds", *Sensors and Actuators B: Chemical*, 1997  
Publication <1 %

---

32 Gupta, V.K.. "Zinc(II)-selective sensors based on dibenzo-24-crown-8 in PVC matrix", *Analytica Chimica Acta*, 20050314  
Publication <1 %

---

33 Ji Hye Kang, Seong Youl Lee, Hye Mi Ahn, Cheal Kim. "A novel colorimetric chemosensor for the sequential detection of Ni<sup>2+</sup> and CN<sup>-</sup> in aqueous solution", *Sensors and Actuators B: Chemical*, 2017  
Publication <1 %

---

34 [epdf.pub](http://epdf.pub)  
Internet Source <1 %

---

35 [hwbdocuments.env.nm.gov](http://hwbdocuments.env.nm.gov)  
Internet Source <1 %

---

36 [tudr.thapar.edu:8080](http://tudr.thapar.edu:8080)  
Internet Source <1 %

---

37

www.amac.md

Internet Source

<1 %

38

Mohammad Reza Ganjali, Parviz Norouzi, Farnoush Faridbod, Nafiseh Hajiabdollah, Rassoul Dinarvand, Soraia Meghdadi. " Lutetium(III) Ions Determination in Biological and Environmental Samples by a Lutetium(III) Sensor Based on ' - bis(2 - Pyridinecarboxamide) - 1,3 - benzene as a Sensing Material ", Analytical Letters, 2008

Publication

<1 %

39

Mojtaba Shamsipur, Mohammad Yousefi, Morteza Hosseini, Mohammad Reza Ganjali. "PVC-BASED 1,3,5-TRITHIANE COATED GRAPHITE ELECTRODE FOR DETERMINATION OF CERIUM(III) IONS", Analytical Letters, 2007

Publication

<1 %

Exclude quotes On

Exclude matches < 3 words

Exclude bibliography On

# Potentiometric Selectivity

GRADEMARK REPORT

FINAL GRADE

**/0**

GENERAL COMMENTS

**Instructor**

PAGE 1

PAGE 2

PAGE 3

PAGE 4