

paper

by Asep Saefurrohman

Submission date: 17-Apr-2023 12:21PM (UTC+0700)

Submission ID: 2066880450

File name: Paper-Template-General.docx (43.87K)

Word count: 2557

Character count: 14708

La(III) ION SELECTIVE ELECTRODE WITH PTFE MEMBRANE CONTAINING TRIBUTYL PHOSPHATE IONOPHORE

Asep Saefurohman^{1,a*}, Buchari^{2,b} and Indra Noviandri^{3,c}

¹Department of Chemistry, The State Islamic University, UIN Sultan Maulana Hasanuddin Banten, Indonesia

²Department of Chemistry, Bandung Institute of Technology, ITB, Indonesia

³Department of Chemistry, Bandung Institute of Technology, ITB, Indonesia

^aasep.saefurohman@uinbanten.ac.id, ^bbuchari@itb.ac.id, ^cinnov@itb.ac.id

Keywords: Lanthanum, electrode selective ion, ionophore.

Introduction

Lanthanum is one of rare earth elements is known as an important element of their nature, especially having a strong magnetic properties. Lanthanum has received much attention electrochemically due to its applications in the hydrogen storage materials of batteries, ion selective electrode, chemical sensor, electrocatalytic hydrogenation, and ion gate effect [1]. It's elements found in nature in the form of minerals such as monazite and xenotime. Monazite and xenotime are minerals that contains lots of rare earth metal element (REE') of the lanthanide group. These mineral also found in Indonesia, but not yet processed and utilized optimally because of the mastery of monazite ore processing technology still needs to be improved and strengthened. REE' these elements, are now widely used for the manufacture of goods innovative high-tech, such as permanent magnets, catalysts, fiber optics, optoelectronics, ceramics piezoelectric, rechargeable batteries, microwave equipment, etc., so that now the element REE has regarded as one of the 21st century [2,3]. Lanthanides are very important metals in high technology industry because of their unique electronic, optical, and magnetic properties, and therefore their demand has been increasing in recent year. But the element of REE' mostly have physical and have very fundamental chemical properties are similar, which makes it difficult hard splitting into each element. It is also the cause of rare earth metals such as lanthanides become expensive [4].

Currently, many researchers who give great attention to rare earth metals are widely applied in industry. Therefore, the required development of method for the determination and recovery of rare earth metals. Method has been developed which includes conventional means such as chemical precipitation, reverse osmosis, adsorption, ion exchange and solvent extraction, but many difficulties are found in a variety of methods [5].

For the purposes of monitoring the treatment process, quality control, and REE' presence in a given material, required analytical methods that have high accuracy and selectivity, low detection limits, and high reproducibility. The method that considered to meet these criteria, among others, spectroscopic techniques such as inductively coupled plasma mass spectrometry (ICPMS), inductively coupled plasma atomic emission spectrometry (ICPAES), and X-ray fluorescence spectrometry. Hence, the available methods for low-level determination of rare-earth ions in solution include spectrophotometry, isotope dilutions mass spectrophotometry, neutron activation analysis, X-ray fluorescence spectrometry, etc [5]. However, many of these spectroscopic methods requires a lot of time involving multiple samples and

also expensive for most analytical laboratories [6]. Meanwhile, if using chromatographic methods require a long sample preparation. Therefore, alternative methods are needed that meet the analytical criteria, simple in execution and relatively inexpensive.

One method that has the potential of the electrode is the potentiometric method with membranous. Potentiometric method provides several advantages such as speed and ease of preparation and procedures, simple instrumentation, relatively fast response, very low detection limits, wide measurement range, an acceptable selectivity and low cost. This will make the availability of micro-electrodes and electrodes for the determination of the required REE [7]. The quick determination of minute quantities of ionic species by simple methods has a great importance in analytical chemistry. Potentiometric detection based on ion selective electrodes (ISEs) is the simplest of all and offers unique advantages [8]. Membranous electrode has many types, and in this paper was chosen with reference to the type of tube and the solution in as well as sensor ionophore required. Therefore, it is feasible the development of methods to make sensors for lanthanide ions with high selectivity using the appropriate ionophore. Electrodes for the potentiometric determination can yield several benefits such as ease and speed of preparation and procedures, simple instrumentation, relatively fast response, wide measurement range and low cost. Therefore, the use of microelectrode and an electrode in the potentiometric analysis REE' is growing. Potentiometric detectors based-on ion selective electrode are specially suited for fast, accurate, reproducible and selective determination of various metal ions. Such potentiometric detectors offer advantages such as selectivity, sensitivity, good precision, simplicity and so on. These methods allow direct on-line monitoring of concentration of selected species without an pretreatment [9].

Carrier-based ion selective electrodes (ISEs) are used extensively for the direct selective detection of ionic species. For this type of electrode, the formation constant of the ion-ionophore complex within the membrane phase is very important parameter that dictates the practical selectivity of the sensor. In the area of membrane based ISEs, emphasis has been focused on the development of new ionophore and on the composition of the membrane phase, aiming at enhancing the potentiometric responses of the ISEs. Fabrication of a new, ion specific ISE with high selectivity and sensitivity, wide linear concentration range, long lifetime, good reproducibility and low cost, is always in need [5,6].

In this paper the compound organophosphates especially TBP will be studied or used as ionophore in membranes in selective electrodes ion. The principle of formation of the measured potential in both surface and transport based on this principle the same as that occurs in the extraction, while the TBP solvent extraction lanthanides have been performed and shown to occur transport from the aqueous phase to organic phase by using TBP. In addition, TBP has not been used as ionophore in potentiometric systems. Hence, to study the character of the membrane on the electrode as a potentiometric sensor, needed characterization, membrane potential, response time, sensitivity, selectivity towards the primary ion and ion bullies are less than 10^{-3} , age (lifetime) is relatively long and has a design size can be miniaturized.

The main objective of this work is to introduce a selective and sensitive electrode for lanthanum, for the potentiometric monitoring of trace amount of La^{3+} , by using TBP as ionophore. In spite of ion selective electrode based on ionophore ligand are well established for many widespread activity in the field of ion selective electrodes during the last two decades, however there is no report previously in the literature TBP as ionophore and its applications for measurement ion La^{3+} .

EXPERIMENTAL PART

1.1 Equipment

All potentiometric measurement were made at $25 \pm 1^\circ\text{C}$ with Ohmeter instrument pH/mV meter. The glass cell, where the La^{3+} ion selective electrode was placed, and a double junction saturated calomel electrode (SCE) was used as internal reference electrode.

1.2 Chemicals and solutions

Tri butyl phosphate were obtained from Sigma Aldrich. Kerosene from sigma Aldrich, PTFE (Advantec, Japan) with pore size $0,45 \mu\text{m}$ and $0,2 \mu\text{m}$. All other reagents used were of analytical grade and the solutions were prepared in doubly distilled water.

2.3 Membrane and Electrode Preparation

The method reported by [8,9,10] was adopted for the fabrication of membranes. Membrane prepared in Impregnated Liquid membrane (ILM). Impregnated Liquid membranes used for prepared ESI-La, with Teflon, length 10 cm, and 1,5 diameter. PTFE (Advantec, Japan) with pore size $0,45 \mu\text{m}$ pore and $0,2 \mu\text{m}$ pore (impregnated in TBP), immersed for 12 and 24 hours respectively. The saturated calomel electrode and the inner solution (a mixture of 10^{-3} M KCl and $10^{-3} \text{ M La}^{3+}$) was set in the tube and connected to coaxial cable. The electrode was conditioned before potentiometric measurement by immersing it into $10^{-3} \text{ M La}_2\text{O}_3$ solution for 12 and 24 hours. A number of membranes of different compositions were prepared and only those which gave reproducible and stable potentials were selected for further studies.

In this study, the electrode was made and prepared in each different conditions (Membrane thickness, concentration of ionophore TBP, concentration of ionic strength adjuster (ISA), Impregnation time, Influence of pH, Life time, limit detection). The potential response of all the three electrode using PTFE membrane $0,45 \mu\text{m}$ pore size with TBP in kerosene was investigated by varying the concentration of the test solution from 1.0×10^{-1} - 1.0×10^{-6} [10].


2.4 Potential Measurement

The potential measurements of the solutions, prepared in the concentration range 1.0×10^{-1} - $1.0 \times 10^{-6} \text{ M La}^{3+}$ ions, were carried out at $25 \pm 1^\circ\text{C}$ with a Metrohm instrument pH/Ion meter. Saturated calomel electrode were employed as reference electrodes and potential were measured by setting up the following assembly:

Internal Reference electrode (SCE) internal solutions Membrane Test Solutions External reference electrode

RESULT AND DISCUSSION


2.1 Working Concentration Range and Slope

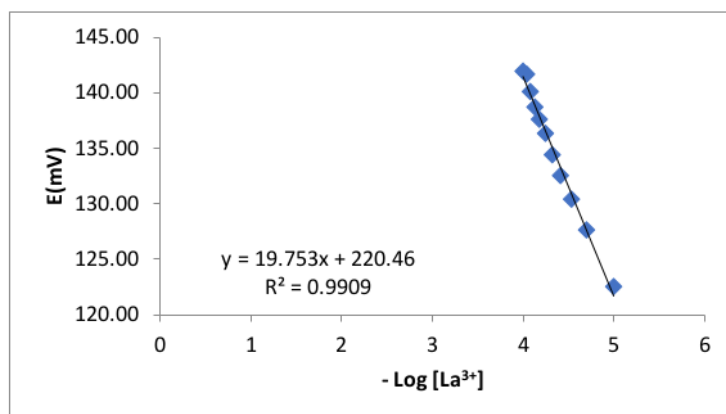

34
Figure 1. The Calibration curve of the La(III) membrane electrode based on TBP

12 2.2 The Effect of pH on the Potential Response

The effect of pH on the potential response of the electrode was studied at different concentration, Standard of 10^{-1} , 10^{-2} , 10^{-3} , 10^{-4} M over the pH range 1-10. A series of solutions of La^{3+} with pH ranging from 1 to 10 were prepared by adding H_2SO_4 and NaOH solutions. Solution potentials were measured by the cell system. pH dependence of the membrane electrode was investigated at 1.0×10^{-3} M La^{3+} concentration in the pH range 1-10 by adjusting the pH solution with H_2SO_4 and NaOH . It was observed that the potential remains constant in the pH range relatively 3-6 and the same was taken as the working pH range of the electrodes. These results indicating the applicability of this electrode in the specific pH range were relatively the same as those reported by other researchers, stating that pH was kept constant at 3-8 [6,7]. On the contrary, relatively noteworthy fluctuations in the potential regarding pH behavior took place below and above the formerly stated pH limit. The fluctuation above the pH value of 6 might be justified by the formation of soluble and insoluble La^{3+} ion hydroxyl complexes in the solution. Hence, the fluctuations below the pH value of 3 were attributed to the partial protonation of the employed ionophore [4]. Considering that deprotonation of the complexes of chelating reagent is one of essential processes for the complex formation. The pH of a sample solutions seem to strongly affect the potentiometric responses. Therefore, influent of protonation and deprotonation complex formation were measured by investigated the pH dependence of the potentiometric responses to the lanthanoid ion.

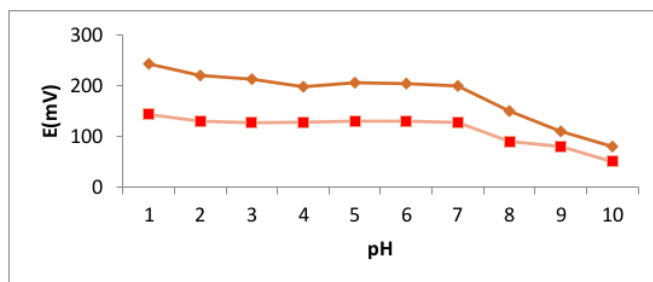

29
Figure 2. Effect of pH on Potential response of ISE-La(III)

The figure 2 above explained correlation between potentiometric response and pH suggest that the potentiometric responses observed with the membrane to the metal ion are induced by the formation of complexes. A typical potential versus pH curve, increasing solution of pH, potential relatively stable and close to Nernstian slope is 19 mV per decade., was observed from pH \approx 7 to 2 both 10^{-2} or 10^{-4} concentration. This pH response suggest that TBP impregnated membrane PTFE at the membrane interface successively protonate with increasing the H^+ concentration of the solution.

The study of sensor properties

The properties of an ion-selective electrode are characterized by parameters like these: measuring range, detection limit, response time, selectivity, stability and life time, reversibility. 40

3.3.1 Measuring range 3

Range measurements, the linear range of the electrode is defined as part of the calibration curve by linear regression which indicates that the data points do not deviate from linearity by more than 2 mV. Range measurements on an ion selective electrode (ISE) including the linear part of the calibration curve. For some electrodes, this range can be expanded from 1 molar to go down 10^{-6} or even 10^{-7} molar. Under other definitions, measurement range of an ion selective electrode is a range of activity between the highest and lowest limits of detection. But recent studies have shown that the range can be reduced to sub-nM detection limit with different methods such as the application of a metal buffer to remove contamination from the aqueous solution, using a cation exchange resin in the internal solution at ISE to keep the main ion activity at a low level constant, uses particles such as silica-gel lipophilic 100 C18 reversed phase into the membrane sensor, using membrane sandwich etc.

3.3.2 Detection limit 35

Limits of detection is determined from the graph the relationship between the potential and the concentration of ions La. Based on the graph, it can be determined the limit of detection by the oblique intersection of straight lines and flat. The limit of detection, as determined from the intersection of the two extrapolated segments of the calibration graph, was 9.2×10^{-6} M.

3.3.3 Response time 2

Dynamic response time is an important factor for an ion selective electrode [1,6]. In this study, the practical response time was recorded by changing solution with different La(III) concentration from 9.9×10^{-6} - 2.06×10^{-4} M. The response time of an electrode is evaluated by measuring the

average time required to achieve a potential within ± 0.1 mV of the final steady-state potential. The response time of the microelectrode was found to be about 20 seconds in the whole concentrations.

CONCLUSIONS 37

In summary, potentiometric selectivity of polymer-membrane electrodes based on lanthanum is one of method used as quantitative analysis of rare earth elements which are considered as the standard method that has a high accuracy, fast response time, and low detection limits. Hence, electrode was prepared by PTFE impregnated membrane in TBP. The Selectivity of ISE-La showed that electrode didn't respond to alkaline elements and transition element but still respond to lanthanide elements such as Ce^{3+} and Nd^{3+}

Acknowledgments

The authors gratefully acknowledge research support from to Ministry of education and culture of Indonesia and I'MHERE Program, faculty mathematic and natural sciences, Institute Technology of Bandung (ITB).

References

- [1] Shou-Qing Liu and Hong yuan Chen. Spectroscopic and voltammetric studies on a lanthanum hexacyanoferrate modified electrode. *Journal of Electroanalytical chemistry*, 528 (2002) 90-195.
- [2] Attas, A. Novel PVC membrane selective electrode for the determination of chlozapine in pharmaceutical preparation. *Int. J. Electrochem. Sci.* 9-19. (2009).
- [3] Morais, CA and Ciminelli, V.S.T. Process development for the recovery of High-grade lanthanum by solvent extraction. *Hydrometallurgy*, **73**, 237- 244.(2004).
- [4] Shimojo, K, Naganawa, H, Noro, J and Kubota, F. Extraction Behavior and separation of lanthanides with a diglycol amic Acid Derivative and a Nitrogen-donor Ligand. *Analytical Sciences*, **23** 1427-1430. (2007).
- [5] Darviche, *et al.* Lanthanide recognition: A Ho^{3+} Potentiometric membrane sensor. *Int. J. Electrochem.Sci.* **3** 1288-1298 (2008).
- [6] Aghaie, *et al.* Tin(II)-Selective membrane potentiometric sensor using a crown ether as neutral carrier. *Sensors and actuators B*. 107 (2004) 756-761).
- [7] Mittal, S.K., Kumar S.K., and Sharma, H.K PVC-Based dicyclohexano-18-crown-6 sensor for La(III) ions. *Talanta* **62** (2004) 801-805.
- [8] Attas, A. Novel PVC membrane selective Electrode for the Determination of Clozapine in Pharmaceutical Preapartions. *Int. J.Electrochem. Sci.* 4 (2009) 9-19.
- [9] Mahajan, R.K, Inderpreet Kaur and Manoj Kumar. Silver ion-selective electrodes employing Schiff base p-tert-butyl calyx[4] arene derivatives as neutral carriers. *Sensor and Actuators B*. 91 26-31. (2003).
- [10] Ganjali M.R., *et al.* Ppt levels detection of samarium (III) with a coated graphite sensor based on an antibiotic, *Analytical Sciences*, **20** (2007) 1007-1011.
- [11] Ganjali, Emami, and Rezapour. Novel gadolinium poly(vinyl chloride) membrane sensor based on a new S-N Sciff's base. *Analytica chimica acta*, **495** (2003) 51-59.

[12] Ajay K. Jain, Vinod K. Gupta, Lok P. Singh, Upendra Khurana. Novel PVC-based membrane sensors selective for vanadyl ions. *Talanta* **46** (1998) 1453–1460.

[13] Ito, K, Goto, C and Noguchi, K. Lanthanoid ion selective solvent polymeric membrane electrode based on 1-phenyl-3-methyl-4-octadecanoyl-5-pyrazolone. *Analytica Chimica Acta*. **443** (2001) 41-51.

Reference to a book:

[1] W.E Morf. The Principles of ion selective electrodes and a membrane transport. Elsevier. New York.1981.

paper

ORIGINALITY REPORT

28%

SIMILARITY INDEX

22%

INTERNET SOURCES

25%

PUBLICATIONS

%

STUDENT PAPERS

PRIMARY SOURCES

1	www.scientific.net Internet Source	1 %
2	anjs.edu.iq Internet Source	1 %
3	James, D.. "Potentiometric sensing of iodide using polymeric membranes of microwave stabilized @b-AgI", <i>Electrochimica Acta</i> , 20120401 Publication	1 %
4	S Mittal. "PVC-based dicyclohexano-18-crown-6 sensor for La(III) ions", <i>Talanta</i> , 2004 Publication	1 %
5	Shou-Qing Liu. "Spectroscopic and voltammetric studies on a lanthanum hexacyanoferrate modified electrode", <i>Journal of Electroanalytical Chemistry</i> , 20020614 Publication	1 %
6	www.orientjchem.org Internet Source	1 %

- | | | |
|----|---|-----|
| 7 | Gupta, V.K.. "Copper(II)-selective potentiometric sensors based on porphyrins in PVC matrix", Sensors & Actuators: B. Chemical, 20060912
Publication | 1 % |
| 8 | Javanbakht, M.. "Cadmium(II)-selective membrane electrode based on a synthesized tetrol compound", Analytica Chimica Acta, 20000309
Publication | 1 % |
| 9 | Somayeh Hashemi, Alireza Nezamzadeh-Ejhieh. "A novel chromium selective electrode based on surfactant-modified Iranian clinoptilolite nanoparticles", Desalination and Water Treatment, 2014
Publication | 1 % |
| 10 | Zamani, H.A.. "A new ytterbium(III) PVC membrane electrode based on 6-methy-4-[[1-(1H-pyrrol-2-yl)methylidene]amino}-3-thioxo-3,4dihydro-1,2,4-triazin-5(2H)-one", Talanta, 20070515
Publication | 1 % |
| 11 | www.science.gov
Internet Source | 1 % |
| 12 | Bholanath Mahanty, A.K. Satpati, P.K. Mohapatra. "Development of a potentiometric sensor for europium(III) based | 1 % |

on N, N, N', N'-tetraoctyldiglycolamide (TODGA) as the ionophore", Journal of Electroanalytical Chemistry, 2018

Publication

13

www.ncbi.nlm.nih.gov

Internet Source

1 %

14

Hassan Ali Zamani, Mahbobeh Mohaddeszadeh. "Determination of Dysprosium(III) Ion in Soil and Sediment Samples by an Original Potentiometric Dysprosium(III) Membrane Sensor", Analytical Letters, 2008

Publication

1 %

15

warwick.ac.uk

Internet Source

1 %

16

www.researchgate.net

Internet Source

1 %

17

Ganjali, M.R.. "Fluoride determination in some mouth wash preparations by a novel La(III) graphite coated membrane sensor based on amitraz", Analytica Chimica Acta, 20050228

Publication

1 %

18

Vinod Kumar Gupta, Lok Pratap Singh, Sudeshna Chandra, Sunita Kumar, Rakesh Singh, Bhavana Sethi. "Anion recognition through amide-based dendritic molecule: A

1 %

poly(vinyl chloride) based sensor for nitrate ion", Talanta, 2011

Publication

19

hysz.nju.edu.cn

Internet Source

1 %

20

Gupta, V.K.. "Porphyrins as carrier in PVC based membrane potentiometric sensors for nickel(II)", Analytica Chimica Acta, 19971120

Publication

1 %

21

Moghim, M.. "Polymeric membrane sensor for potentiometric determination of vanadyl ions", Analytica Chimica Acta, 20041206

Publication

1 %

22

S. Dian Siti, Ihsanawati, Rukman Hertadi. "Isolation and Characterization of Organic-Solvent Stable Protease Isolated by Pseudomonas stutzeri BK AB-12", Procedia Chemistry, 2015

Publication

1 %

23

acta.chem-soc.si

Internet Source

1 %

24

Faridbod, F.. "Multi-walled carbon nanotubes (MWCNTs) and room temperature ionic liquids (RTILs) carbon paste Er(III) sensor based on a new derivative of dansyl chloride", Electrochimica Acta, 20091215

Publication

1 %

25 M. Aghaie, M. Giahi, M. Zawari. <1 %
"Manganese(II) Ion-Selective Membrane
Electrode Based on N-(2-picolinamido ethyl)-
Picolinamide as Neutral Carrier", Bulletin of
the Korean Chemical Society, 2010
Publication

26 ijasjournal.org <1 %
Internet Source

27 staff.uny.ac.id <1 %
Internet Source

28 www.csass.org <1 %
Internet Source

29 Ahmed A. Abdel Gaber. "A Novel PVC
Membrane Sensor for Selective
Determination of Cerium(III) Ions", Analytical
Letters, 2003
Publication

30 Alizadeh, N.. "Linear alkylbenzenesulfonate
(LAS) ion-selective electrode based on
electrochemically prepared polypyrrole and
PVC", Sensors & Actuators: B. Chemical,
20010430
Publication

31 Mehran Ghiaci, Behzad Rezaei, Zahra Sadeghi,
Javad Safaei-Ghomi. " A Co -Selective
Poly(vinyl chloride) Membrane Electrode
Based on a Newly Synthesized 3,3'-

(Dodecylazanediy)bis(-(2-(2-aminoethylamino)ethyl)propanamide) Compound ", Journal of Chemical & Engineering Data, 2010

Publication

32

journal.islamiconomic.or.id

Internet Source

<1 %

33

www.peacta.org

Internet Source

<1 %

34

Ganjali, M.R.. "Fabrication of a highly selective Eu(III) membrane sensor based on a new S-N hexadentates Schiff's base", Sensors & Actuators: B. Chemical, 20070110

Publication

<1 %

35

Mohammad Reza Ganjali, Vinod Kumar Gupta, Morteza Hosseini, Maryam Hariri, Farnoush Faridbod, Parviz Norouzi. "Lanthanide recognition: A dysprosium(III) selective fluorimetric bulk optode", Sensors and Actuators B: Chemical, 2012

Publication

<1 %

36

jbcs.s bq.org.br

Internet Source

<1 %

37

www.iosrjournals.org

Internet Source

<1 %

38

www.omicsonline.org

Internet Source

<1 %

39

Mohamed B. Saleh, Ezzat M. Soliman, Ahmed A. Abdel Gaber, Salwa A. Ahmed. "A Novel Hg(II) PVC Membrane Sensor Based on Simple Ionophore Ethylenediamine Bis - Thiophenecarboxaldehyde", Analytical Letters, 2006

Publication

<1 %

40

Mohammad Reza Ganjali, Vinod Kumar Gupta, Farnoush Faridbod, Parviz Norouzi. "Electrochemical Determination of Lanthanides Series", Elsevier BV, 2016

Publication

<1 %

41

Vinod K Gupta. "A PVC-based 12-crown-4 membrane potentiometric sensor for zinc (II) ions", Sensors and Actuators B: Chemical, 1999

Publication

<1 %

42

worldwidescience.org

Internet Source

<1 %

43

www.bcc.bas.bg

Internet Source

<1 %

44

Kenneth N. Han, Jon J. Kellar, William M. Cross, Sadegh Safarzadeh. "Opportunities and challenges for treating rare-earth elements", Geosystem Engineering, 2014

Publication

<1 %

45

Singh, A.K.. "A bromide selective polymeric membrane electrode based on Zn(II) macrocyclic complex", Talanta, 20060715

Publication

<1 %

Exclude quotes On

Exclude matches < 3 words

Exclude bibliography On

paper

GRADEMARK REPORT

FINAL GRADE

/0

GENERAL COMMENTS

Instructor

PAGE 1

PAGE 2

PAGE 3

PAGE 4

PAGE 5

PAGE 6

PAGE 7
